

TruSeq™ Small RNA

Sample Preparation Guide

FOR RESEARCH USE ONLY

Introduction	3
Sample Prep Workflow	5
Best Practices	6
RNA Input Recommendations	7
Pooling	8
Kit Contents	9
Consumables and Equipment	15
Ligate 3' and 5' Adapters	17
Reverse Transcribe and Amplify	20
Purify cDNA Construct	26
Validate the Library	32
DNA Template Storage	33
Indexes	34
Technical Assistance	35

This document and its contents are proprietary to Illumina, Inc. and its affiliates ("Illumina"), and are intended solely for the contractual use of its customer in connection with the use of the product(s) described herein and for no other purpose. This document and its contents shall not be used or distributed for any other purpose and/or otherwise communicated, disclosed, or reproduced in any way whatsoever without the prior written consent of Illumina. Illumina does not convey any license under its patent, trademark, copyright, or common-law rights nor similar rights of any third parties by this document.

The instructions in this document must be strictly and explicitly followed by qualified and properly trained personnel in order to ensure the proper and safe use of the product(s) described herein. All of the contents of this document must be fully read and understood prior to using such product(s).

FAILURE TO COMPLETELY READ AND EXPLICITLY FOLLOW ALL OF THE INSTRUCTIONS CONTAINED HEREIN MAY RESULT IN DAMAGE TO THE PRODUCT(S), INJURY TO PERSONS, INCLUDING TO USERS OR OTHERS, AND DAMAGE TO OTHER PROPERTY.

ILLUMINA DOES NOT ASSUME ANY LIABILITY ARISING OUT OF THE IMPROPER USE OF THE PRODUCT(S) DESCRIBED HEREIN (INCLUDING PARTS THEREOF OR SOFTWARE) OR ANY USE OF SUCH PRODUCT(S) OUTSIDE THE SCOPE OF THE EXPRESS WRITTEN LICENSES OR PERMISSIONS GRANTED BY ILLUMINA IN CONNECTION WITH CUSTOMER'S ACQUISITION OF SUCH PRODUCT(S).

FOR RESEARCH USE ONLY

© 2010 Illumina, Inc. All rights reserved.

Illumina, illuminaDx, Solexa, Making Sense Out of Life, Oligator, Sentrix, GoldenGate, GoldenGate Indexing, DASL, BeadArray, Array of Arrays, Infinium, BeadXpress, VeraCode, IntelliHyb, iSelect, CPro, GenomeStudio, Genetic Energy, HiSeq, HiScan, Eco, and TruSeq are registered trademarks or trademarks of Illumina, Inc. All other brands and names contained herein are the property of their respective owners.

Phusion is a trademark of Finnzymes Oy.


Notice to Purchaser: Limited license (proofreading DNA polymerases). The purchase price of this product includes a limited, non-transferable license under U.S. and foreign patents (5,500,363 and 5,352,778) owned by New England Biolabs, Inc. to use this product. No other license under these patents is conveyed expressly or by implication to the purchaser by the purchase of this product. The purchase price of this product includes a limited, non-transferable license under U.S. and foreign patents owned by BIO-RAD Laboratories, Inc., to use this product. No other license under these patents is conveyed expressly or by implication to the purchaser by the purchase of this product.

Introduction

The Illumina® TruSeq™ Small RNA Sample Preparation protocol is used to prepare a variety of RNA species. The protocol takes advantage of the natural structure common to most known microRNA molecules. Most mature miRNAs have a 5'-phosphate and a 3'-hydroxyl group as a result of the cellular pathway used to create them. Because of this, the Illumina adapters in this kit are directly, and specifically, ligated to miRNAs.

This guide explains how to prepare libraries for subsequent cluster generation, using total RNA or purified small RNA as input. The protocol describes the steps for adapter ligation, reverse transcription, PCR amplification, and pooled gel purification to generate a library product.

Figure 1 Fragments after TruSeq Small RNA Sample Preparation

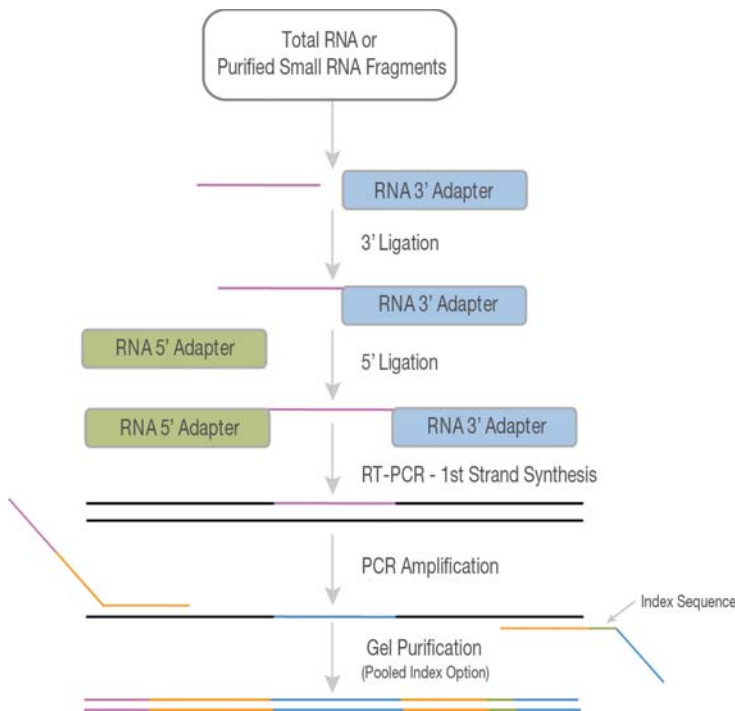

The RNA 3' adapter is specifically modified to target microRNAs and other small RNAs that have a 3' hydroxyl group resulting from enzymatic cleavage by Dicer or other RNA processing enzymes. The adapters are ligated to each end of the RNA molecule and an RT reaction is used to create single stranded cDNA. The cDNA is then PCR amplified using a common primer and a primer containing one of 48 index sequences. The introduction of the index sequence at the PCR step separates the indexes from the RNA ligation reaction. This design allows for the indexes to be read using a second read and significantly reduces bias compared to designs which include the index within the first read.

One feature of the TruSeq Small RNA Sample Preparation protocol is to allow use of 48 different index tags to make use of the Illumina multiplexing capability for analysis of directional and small RNA samples (see *Indexes* on page 34). The Illumina multiplexing system employs six-base indices to distinguish different samples from one another in a single lane of a flowcell. The kits are configured for 24 reactions with 12 different indexes per kit. The 48 indexes are divided into four different kits:

Table 1 TruSeq Small RNA Sample Prep Kits


Indices	Catalog #	Contains Core Solutions Box and Indices Box:
1–12	RS-200-0012	A
13–24	RS-200-0024	B
25–36	RS-200-0036	C
37–48	RS-200-0048	D

Sample Prep Workflow

The following diagram illustrates a single TruSeq Small RNA Sample Preparation workflow. For multiplexing libraries, all samples are processed in parallel through the RT-PCR Amplification process. After PCR amplification, libraries from separate samples can be pooled for a single gel isolation.

Figure 2 TruSeq Small RNA Sample Preparation Workflow

Day 1

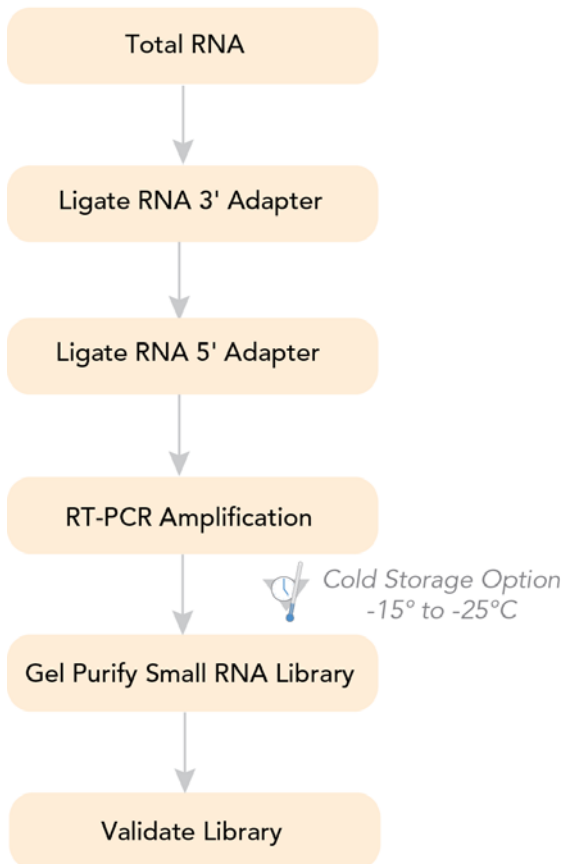

Best Practices

RNA is highly susceptible to degradation by RNase enzymes. RNase enzymes are present in cells and tissues, and carried on hands, labware, and dust. They are very stable and difficult to inactivate. For these reasons, it is important to follow best laboratory practices while preparing and handling RNA samples.

- ▶ When harvesting total RNA, use a method that quickly disrupts tissue and isolates and stabilizes RNA.
- ▶ Wear gloves and use sterile technique at all times.
- ▶ Reserve a set of pipettes for RNA work. Use sterile RNase-free filter pipette tips to prevent cross-contamination.
- ▶ Use disposable plasticware that is certified to be RNase-free. Illumina recommends the use of non-sticky sterile RNase-free microcentrifuge tubes. These should not be used for other lab work.
- ▶ All reagents should be prepared from RNase-free components, including ultra pure water.
- ▶ Store RNA samples by freezing. Keep samples on ice at all times while working with them. Avoid extended pauses in the protocol until the RNA is in the form of double-stranded DNA.
- ▶ Use RNase/DNase decontamination solution to decontaminate work surfaces and equipment prior to starting this protocol.

RNA Input Recommendations

Total RNA Input

This protocol has been optimized using 1 µg of high-quality human or mouse brain total RNA as input. Small RNA populations can vary significantly between different tissue types and species. Use of RNA from other species, tissues, or qualities may require further optimization with regard to the initial input amount and selection of the desired bands during the final gel excision. The types and coverage of small RNAs sequenced will also vary depending on which bands are selected during gel excision.

It is very important to use high-quality RNA as the starting material. Use of degraded RNA can result in low yield or failure of the protocol. Illumina recommends that you check total RNA integrity following isolation using an Agilent Technologies 2100 Bioanalyzer with an RNA Integrity Number (RIN) value greater than 8.

Alternatively, you can run a formaldehyde 1% agarose gel and judge the integrity of RNA upon staining with ethidium bromide. High quality human RNA will show a 28S rRNA band at 4.5 kb that should be twice the intensity of the 18S rRNA band at 1.9 kb. Both kb determinations are relative to a RNA 6000 ladder. The mRNA will appear as a smear from 0.5–12 kb.

Purified Small RNA Input

You can also use previously isolated micro RNA as starting material. Use the entire fraction of small RNA purified from 1–10 µg of total RNA. Fewer undesired bands will be seen during the subsequent gel extraction using this method.



NOTE

Purified small RNAs *must* be in molecular grade water or 10 mM Tris buffer.

Positive Control

Illumina recommends using Ambion FirstChoice human brain total RNA (catalog # AM7962) as a positive control sample for this protocol. This preparation is certified to contain the small RNA fraction.

Pooling

The TruSeq Small RNA Sample Preparation kit can be used to construct libraries that are compatible with Illumina multiplexing, with up to 48 samples combined into a single lane. While processing samples in parallel, incorporate the index at the amplification step following reverse transcription. Pool samples immediately prior to gel purification, or after gel purification and library validation. Pooling prior to gel purification can greatly reduce the number of necessary gel purifications.

Pool libraries in equimolar amounts. However, determining library concentrations before gel purification can be challenging. The Agilent Bioanalyzer High Sensitivity DNA chip offers an estimate of library concentration if the peaks corresponding to the amplified small RNA species can be distinguished and quantified.

Libraries can also be pooled prior to gel purification using equal small volumes. The volume of each sample that is pooled depends on the number of samples being pooled, with the total volume of a pool being 50 μ l before gel purification. For example, a pool of 12 samples would use 4 μ l each, a pool of 24 samples would use 2 μ l each, and a pool of 48 samples would use 1 μ l each. These pools would be loaded into two lanes of the PAGE gel.

Different biological samples can have widely varying levels of small RNA. Pooling by volume gives better results with samples derived from similar species and tissues. In the case of highly-multiplexed runs, if necessary, repool and resequence any samples that do not provide sufficient coverage.

Kit Contents


Check to ensure that you have all of the TruSeq Small RNA Sample Prep reagents identified in this section before proceeding. You will receive one TruSeq Small RNA Sample Prep Core Solutions box (24 samples) and one TruSeq Small RNA Sample Prep Indices box (A, B, C, or D) per TruSeq Small RNA Sample Prep Kit (see Table 1 on page 4).

Core Solutions, Box Contents

Store at -15° to -25°C

This box is shipped on dry ice. As soon as you receive it, store the following components at -15° to -25°C .

Figure 3 TruSeq Small RNA Sample Prep Core Solutions Box, part # 15016911

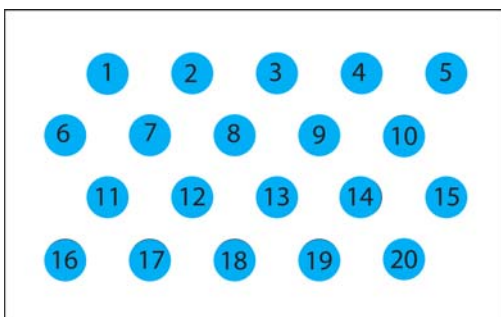

- 1 Custom RNA Ladder, part # 15019413
- 2 5X HM Ligation Buffer (HML), part # 15013206
- 3 Stop Solution (STP), part # 15016304
- 4 T4 RNA Ligase, part # 1000587
- 5 RNase Inhibitor, part # 15003548
- 6 RNase Inhibitor, part # 15003548
- 7 10 mM ATP, part # 15007432
- 8 5X Phusion™ HF Buffer (Finnzymes Oy), part # 1000585
- 9 5X Phusion HF Buffer (Finnzymes Oy), part # 1000585
- 10 Phusion Polymerase (Finnzymes Oy), part # 1000584


- 11 Phusion Polymerase (Finnzymes Oy), part # 1000584
- 12 25 mM dNTP Mix, part # 11318102
- 13 High Resolution Ladder, part # 15019401
- 14 10X Gel Elution Buffer, part # 1000571
- 15 Glycogen, part # 15009052
- 16 Ultra Pure Water, part # 1001913
- 17 Ultra Pure Water, part # 1001913
- 18 Ultra Pure Water, part # 1001913
- 19 Ultra Pure Water, part # 1001913
- 20 Resuspension Buffer, part # 1001388

Indices A, Box Contents

Store at -15° to -25°C

This box is shipped on dry ice. As soon as you receive it, store the following components at -15° to -25°C.

Figure 4 TruSeq Small RNA Sample Prep Indices A Box, part # 15016912

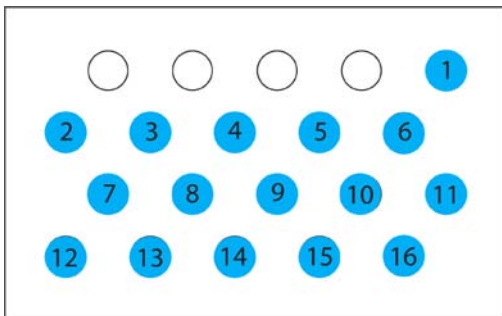

- 1 RNA RT Primer (RTP), part # 15013981
- 2 RNA 3' Adapter (RA3), part # 15013207
- 3 RNA 5' Adapter (RA5), part # 15013205
- 4 RNA PCR Primer (RP1), part # 15005505
- 5 RNA PCR Primer Index 1 (RPI1), part # 15013181


- 6 RNA PCR Primer Index 2 (RPI2), part # 15013185
- 7 RNA PCR Primer Index 3 (RPI3), part # 15013186
- 8 RNA PCR Primer Index 4 (RPI4), part # 15013187
- 9 RNA PCR Primer Index 5 (RPI5), part # 15013188
- 10 RNA PCR Primer Index 6 (RPI6), part # 15013189
- 11 RNA PCR Primer Index 7 (RPI7), part # 15013190
- 12 RNA PCR Primer Index 8 (RPI8), part # 15013191
- 13 RNA PCR Primer Index 9 (RPI9), part # 15013192
- 14 RNA PCR Primer Index 10 (RPI10), part # 15013193
- 15 RNA PCR Primer Index 11 (RPI11), part # 15013195
- 16 RNA PCR Primer Index 12 (RPI12), part # 15013196

Indices B, Box Contents

Store at -15° to -25°C

This box is shipped on dry ice. As soon as you receive it, store the following components at -15° to -25°C.

Figure 5 TruSeq Small RNA Sample Prep Indices B Box part # 15016914

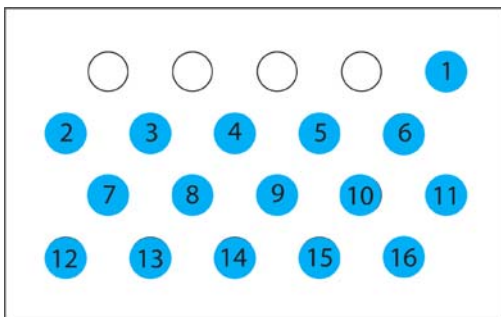

- 1 RNA RT Primer (RTP), part # 15013981
- 2 RNA 3' Adapter (RA3), part # 15013207
- 3 RNA 5' Adapter (RA5), part # 15013205
- 4 RNA PCR Primer (RP1), part # 15005505


- 5 RNA PCR Primer Index 13 (RPI13), part # 15016268
- 6 RNA PCR Primer Index 14 (RPI14), part # 15016269
- 7 RNA PCR Primer Index 15 (RPI15), part # 15016270
- 8 RNA PCR Primer Index 16 (RPI16), part # 15016271
- 9 RNA PCR Primer Index 17 (RPI17), part # 15016272
- 10 RNA PCR Primer Index 18 (RPI18), part # 15016273
- 11 RNA PCR Primer Index 19 (RPI19), part # 15016274
- 12 RNA PCR Primer Index 20 (RPI20), part # 15016275
- 13 RNA PCR Primer Index 21 (RPI21), part # 15016276
- 14 RNA PCR Primer Index 22 (RPI22), part # 15016277
- 15 RNA PCR Primer Index 23 (RPI23), part # 15016278
- 16 RNA PCR Primer Index 24 (RPI24), part # 15016279

Indices C, Box Contents

Store at -15° to -25°C

This box is shipped on dry ice. As soon as you receive it, store the following components at -15° to -25°C .

Figure 6 TruSeq Small RNA Sample Prep Indices C Box, part # 15016916

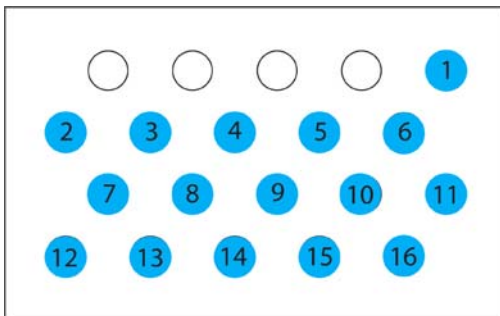

- 1 RNA RT Primer (RTP), part # 15013981
- 2 RNA 3' Adapter (RA3), part # 15013207
- 3 RNA 5' Adapter (RA5), part # 15013205


- 4 RNA PCR Primer (RP1), part # 15005505
- 5 RNA PCR Primer Index 25 (RPI25), part # 15016280
- 6 RNA PCR Primer Index 26 (RPI26), part # 15016281
- 7 RNA PCR Primer Index 27 (RPI27), part # 15016282
- 8 RNA PCR Primer Index 28 (RPI28), part # 15016283
- 9 RNA PCR Primer Index 29 (RPI29), part # 15016284
- 10 RNA PCR Primer Index 30 (RPI30), part # 15016285
- 11 RNA PCR Primer Index 31 (RPI31), part # 15016286
- 12 RNA PCR Primer Index 32 (RPI32), part # 15016287
- 13 RNA PCR Primer Index 33 (RPI33), part # 15016288
- 14 RNA PCR Primer Index 34 (RPI34), part # 15016289
- 15 RNA PCR Primer Index 35 (RPI35), part # 15016290
- 16 RNA PCR Primer Index 36 (RPI36), part # 15016291

Indices D, Box Contents

Store at -15° to -25°C

This box is shipped on dry ice. As soon as you receive it, store the following components at -15° to -25°C .

Figure 7 TruSeq Small RNA Sample Prep Indices D Box, part # 15016918

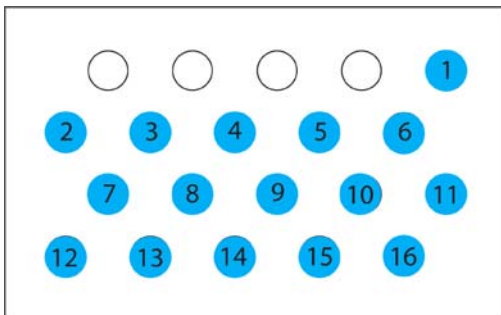

- 1 RNA RT Primer (RTP), part # 15013981
- 2 RNA 3' Adapter (RA3), part # 15013207

- 3 RNA 5' Adapter (RA5), part # 15013205
- 4 RNA PCR Primer (RP1), part # 15005505
- 5 RNA PCR Primer Index 37 (RPI37), part # 15016292
- 6 RNA PCR Primer Index 38 (RPI38), part # 15016293
- 7 RNA PCR Primer Index 39 (RPI39), part # 15016294
- 8 RNA PCR Primer Index 40 (RPI40), part # 15016295
- 9 RNA PCR Primer Index 41 (RPI41), part # 15016296
- 10 RNA PCR Primer Index 42 (RPI42), part # 15016298
- 11 RNA PCR Primer Index 43 (RPI43), part # 15016298
- 12 RNA PCR Primer Index 44 (RPI44), part # 15016299
- 13 RNA PCR Primer Index 45 (RPI45), part # 15016300
- 14 RNA PCR Primer Index 46 (RPI46), part # 15016301
- 15 RNA PCR Primer Index 47 (RPI47), part # 15016302
- 16 RNA PCR Primer Index 48 (RPI48), part # 15016303

Consumables and Equipment

Check to ensure that you have all of the necessary user-supplied consumables and equipment before proceeding to TruSeq Small RNA Sample Preparation.

Table 2 User-Supplied Consumables

Consumable	Supplier
0.2 ml, 1.5 ml, and 2 ml clean, nuclease-free microcentrifuge tubes	General lab supplier (e.g., IST Engineering, VWR, Eppendorf, Fisher Scientific) IST Engineering, 2 ml tube part # 5488-100
1 µg Total RNA in 5 µl nuclease-free water	User experimental samples
3 M NaOAc, pH 5.2	General lab supplier
5 µm filter tube	IST Engineering, part # 5388-50 www.isteng.com/biotech.asp
5X Novex TBE buffer	Invitrogen, part # LC6675
6% Novex TBE PAGE gel, 1.0 mm, 10 well	Invitrogen, part # EC6265BOX
200 µl, clean, nuclease-free PCR tubes	General lab supplier
Clean scalpels	General lab supplier
DNA 1000 chip	Agilent, part # 5067-1504
DNA loading dye	Invitrogen, part # LC6678 or equivalent
Ethanol 100%, -15° to -25°C	General lab supplier
Ethanol 70%, room temperature	General lab supplier
Gel Breaker tube	IST Engineering, part # 3388-100 www.isteng.com/biotech.asp
High Sensitivity DNA chip	Agilent, part # 5067-4626
SuperScript II reverse transcriptase with 100 mM DTT and 5X first strand buffer	Invitrogen, part # 18064-014

Table 2 User-Supplied Consumables (Continued)

Consumable	Supplier
T4 RNA Ligase 2, truncated	NEB, part # M0242S
Ultra pure ethidium bromide 10 mg/ml	General lab supplier
[Optional] Pellet Paint NF Co-Precipitant	Novagen, part # 70748
[Optional] Positive control RNA	Ambion, catalog # AM7962 or equivalent

Table 3 User-Supplied Equipment

Equipment	Supplier
37°C heat block	General lab supplier
4°C microcentrifuge (for ethanol precipitation)	General lab supplier
96-well working rack for 200 µl tubes	Stratagene, part # 410094 or equivalent
Benchtop microcentrifuge	General lab supplier
Bioanalyzer	Agilent
Dark Reader transilluminator or UV transilluminator	Clare Chemical Research, part # D195M
Electrophoresis power supply	General lab supplier
Room temperature tube rotator	General lab supplier
Thermal cycler	General lab supplier
XCell Sure Lock Mini-Cell electrophoresis unit	Invitrogen, part # EI0001

Ligate 3' and 5' Adapters

This process describes the sequential ligation of the RNA 3' and RNA 5' RNA adapters to the sample.

Illumina-Supplied Consumables

- ▶ 5X HM Ligation Buffer (HML)
- ▶ 10 mM ATP
- ▶ RNA 3' Adapter (RA3)
- ▶ RNA 5' Adapter (RA5)
- ▶ RNase Inhibitor
- ▶ Stop Solution (STP)
- ▶ T4 RNA Ligase
- ▶ Ultra Pure Water

User-Supplied Consumables

- ▶ T4 RNA Ligase 2, Truncated



NOTE

It is important to use a 96-well working rack when handling 200 μ l PCR tubes on ice.

Preparation

- ▶ Remove the Illumina-supplied consumables from -15° to -25°C storage and thaw on ice.
- ▶ Briefly centrifuge the thawed Illumina-supplied consumables at 3,000 rpm for 5 seconds, then place them on ice.
- ▶ Pre-heat the thermal cycler to 70°C .

Ligate 3' Adapter

- 1 Set up the ligation reaction in a sterile, nuclease-free 200 μ l PCR tube on ice using the following:

Reagent	Volume (μ l)
RNA 3' Adapter (RA3)	1
1 μ g Total RNA in Nuclease-free Water	5
Total Volume	6

- 2 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly.
- 3 Incubate the tube on the pre-heated thermal cycler at 70°C for 2 minutes and then immediately place the tube on ice.



NOTE

It is very important to keep the RNA 3' Adapter on ice after the 70°C incubation to prevent secondary structure formation.

- 4 Pre-heat the thermal cycler to 28°C.
- 5 Prepare the following mix in a separate, sterile, nuclease-free 200 μ l PCR tube on ice. Multiply each reagent volume by the number of samples being prepared. Make 10% extra reagent if you are preparing multiple samples.

Reagent	Volume (μ l)
5X HM Ligation Buffer (HML)	2
RNase Inhibitor	1
T4 RNA Ligase 2, truncated	1
Total Volume	4

- 6 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly.

- 7 Add 4 μl of the mix to the reaction tube from step 1 and gently pipette the entire volume up and down 6–8 times to mix thoroughly. The total volume of the reaction should be 10 μl .
- 8 Incubate the tube on the pre-heated thermal cycler at 28°C for 1 hour.
- 9 With the reaction tube remaining on the thermal cycler, add 1 μl Stop Solution (STP) and gently pipette the entire volume up and down 6–8 times to mix thoroughly. Continue to incubate the reaction tube on the thermal cycler at 28°C for 15 minutes, and then place the tube on ice.

Ligate 5' Adapter

- 1 Pre-heat the thermal cycler to 70°C.
- 2 Aliquot 1.1 x N μl of the RNA 5' Adapter (RA5) into a separate, nuclease-free 200 μl PCR tube, with N equal to the number of samples being processed for the current experiment.
- 3 Incubate the adapter on the pre-heated thermal cycler at 70°C for 2 minutes and then immediately place the tube on ice.



NOTE

It is very important to keep the RNA 5' Adapter on ice after the 70°C incubation to prevent secondary structure formation. When handling the RNA 5' RNA Adapter, pipette from one tube on ice to another tube on ice and pipette mix the reactions.

- 4 Pre-heat the thermal cycler to 28°C.
- 5 Add 1.1 X N μl of 10mM ATP to the aliquoted RNA 5' Adapter tube, with N equal to the number of samples being processed for the current experiment. Gently pipette the entire volume up and down 6–8 times to mix thoroughly.
- 6 Add 1.1 X N μl of T4 RNA Ligase to the aliquoted RNA 5' Adapter tube, with N equal to the number of samples being processed for the current experiment. Gently pipette the entire volume up and down 6–8 times to mix thoroughly.
- 7 Add 3 μl of the mix from the aliquoted RNA 5' Adapter tube to the reaction from step 9 of *Ligate 3' Adapter*. Gently pipette the entire volume up and down 6–8 times to mix thoroughly.
The total volume of the reaction should now be 14 μl .
- 8 Incubate the reaction tube on the pre-heated thermal cycler at 28°C for 1 hour and then place the tube on ice.

Reverse Transcribe and Amplify

Reverse transcription followed by PCR is used to create cDNA constructs based on the small RNA ligated with 3' and 5' adapters. This process selectively enriches those fragments that have adapter molecules on both ends. PCR is performed with two primers that anneal to the ends of the adapters.

Illumina-Supplied Consumables

- ▶ 5X Phusion HF Buffer (Finnzymes Oy)
- ▶ 25 mM dNTP Mix
- ▶ Phusion Polymerase (Finnzymes Oy)
- ▶ RNA PCR Primer (RP1)
- ▶ RNA PCR Primer Index (1–48) (RPI1–RPI48)
(1 tube of each, depending on the RNA PCR Primer Indices being used)
- ▶ RNA RT Primer (RTP)
- ▶ RNase Inhibitor
- ▶ Ultra Pure Water

User-Supplied Consumables

- ▶ 5' and 3' Adapter-ligated RNA (6 μ l)
- ▶ 5X First Strand Buffer
- ▶ 100 mM DTT
- ▶ High Sensitivity DNA Chip
- ▶ SuperScript II Reverse Transcriptase



NOTE

The TruSeq Small RNA Sample Prep Kits contain up to 48 different Indexed PCR primers, each with a different index. During the PCR step, RNA PCR Primer is used with every library with only one of the 48 RNA PCR Primer Indices per library.

Preparation

- ▶ Remove the Illumina-supplied consumables from -15° to -25°C storage and thaw on ice.
- ▶ Briefly centrifuge the thawed Illumina-supplied consumables at 3,000 rpm for 5 seconds, then place them on ice.
- ▶ Pre-heat the thermal cycler to 70°C .

Dilute 25 mM dNTP Mix

- 1 Dilute the 25 mM dNTPs by premixing the following reagents in a separate, sterile, nuclease-free, 200 μ l PCR tube. Multiply each reagent volume by the number of samples being prepared. Make 10% extra reagent if you are preparing multiple samples.

Reagent	Volume (μ l)
25 mM dNTP mix	0.5
Ultra Pure Water	0.5
Total Volume per Sample	1.0

- 2 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly.
- 3 Label the tube “12.5 mM dNTP Mix” and then place it on ice.

Perform Reverse Transcription

- 1 Combine the following in a separate, sterile, nuclease-free, 200 μ l PCR tube.

Reagent	Volume (μ l)
5' and 3' Adapter-ligated RNA	6
RNA RT Primer (RTP)	1
Total Volume per Sample	7



NOTE

The remaining 5' and 3' adapter-ligated RNA may be stored at -80°C .

- 2 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly.
- 3 Incubate the tube on the pre-heated thermal cycler at 70°C for 2 minutes and then immediately place the tube on ice.

- 4 Pre-heat the thermal cycler to 50°C.
- 5 Prepare the following mix in a separate, sterile, nuclease-free, 200 µl PCR tube placed on ice. Multiply each reagent volume by the number of samples being prepared. Make 10% extra reagent if you are preparing multiple samples.

Reagent	Volume (µl)
5X First Strand Buffer	2
12.5 mM dNTP mix	0.5
100 mM DTT	1
RNase Inhibitor	1
SuperScript II Reverse Transcriptase	1
Total Volume per Sample	5.5

- 6 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly.
- 7 Add 5.5 µl of the mix to the reaction tube from step 3. Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly. The total volume should now be 12.5 µl.
- 8 Incubate the tube in the pre-heated thermal cycler at 50°C for 1 hour and then place the tube on ice.

Perform PCR Amplification

- 1 Prepare the PCR master mix for each index used, in the following order, in a separate, sterile, nuclease-free, 200 μ l PCR tube placed on ice. Multiply each reagent volume by the number of samples being prepared. Make 10% extra reagent if you are preparing multiple samples.

Reagent	Volume (μ l)
Ultra Pure Water	22.5
5X Phusion HF Buffer	10
RNA PCR Primer (RP1)	2
RNA PCR Primer Index (RPIX)	2
25 mM dNTP	0.5
Phusion DNA Polymerase	0.5
Total Volume per Sample	37.5



NOTE

For each reaction, only one of the 48 RNA PCR Primer Indices is used during the PCR step.

- 2 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly, then place the tube on ice.
- 3 Add 37.5 μ l of PCR master mix to the reaction tube from step 8 of *Perform Reverse Transcription*.
- 4 Gently pipette the entire volume up and down 6–8 times to mix thoroughly, then centrifuge briefly and place the tube on ice.
The total volume should now be 50 μ l.

- 5 Amplify the tube in the thermal cycler using the following PCR cycling conditions:
 - a 30 seconds at 98°C
 - b 11 cycles of:
 - 10 seconds at 98°C
 - 30 seconds at 60°C
 - 15 seconds at 72°C
 - c 10 minutes at 72°C
 - d Hold at 4°C
- 6 Run each sample on a high sensitivity DNA chip according to the manufacturer's instructions. The following figure shows typical results from human brain total RNA.



NOTE


Amplification products may vary based on RNA input amount, tissue type, and species. This process was optimized using 1 µg of total RNA from mouse and human brain. The number of PCR cycles can be adjusted, to a maximum of 15 cycles, if clear and distinct bands are not observed in the gel image.



NOTE

The bands of the high sensitivity chip can shift from sample to sample due to an incorrect identification of the marker by the Bioanalyzer software.

Figure 8 Human Brain Total RNA Sample Trace of Amplicons on High Sensitivity DNA Chip

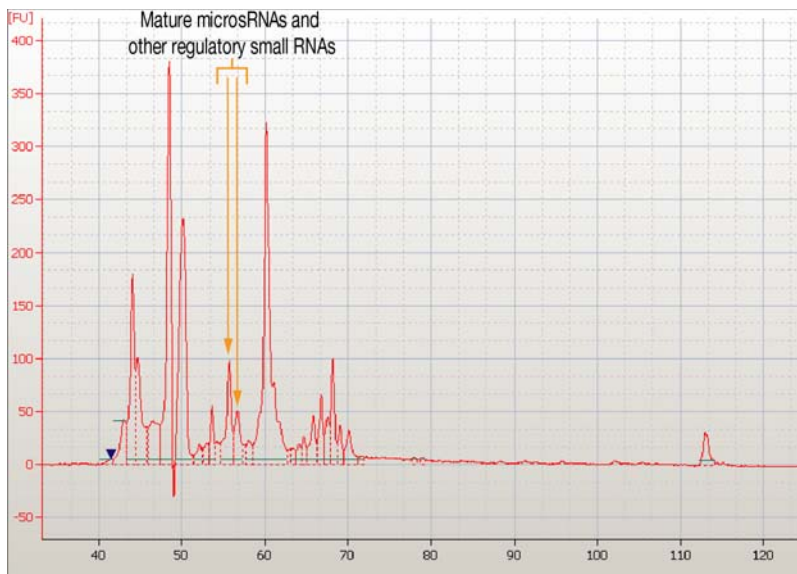

SAFE STOPPING POINT

If you do not plan to proceed to Purify cDNA Construct immediately, the protocol can be safely stopped here. If you are stopping, store the samples at -15° to -25°C overnight or longer. When proceeding, thaw the samples on ice.

Purify cDNA Construct

This process gel purifies the amplified cDNA construct in preparation for subsequent cluster generation.

At this point in the protocol, individual libraries with unique indices may be pooled and gel purified together. Combine equal volumes of the library or molar amounts and then load the samples on the gel according to the instructions below. Do not load more than 30 μ l of sample per well.



NOTE

It is important to follow this procedure exactly to ensure reproducibility.



NOTE

The workflow for pooling more than three samples becomes advantageous to pool by volume. In testing, using the same sample type, a 25% CV of reads per index was achieved.



CAUTION

Illumina does not recommend purifying multiple samples containing the same index on a single gel due to the risk of cross-contamination between libraries. If multiple samples are run on a single gel, keep at least four empty wells between samples.

Illumina-Supplied Consumables

- ▶ 10X Elution Buffer
- ▶ Custom Ladder
- ▶ High Resolution Ladder
- ▶ Glycogen
- ▶ Resuspension Buffer
- ▶ Ultra Pure Water

User-Supplied Consumables

- ▶ Gel Breaker Tubes
- ▶ 3 M NaOAc, pH 5.2
- ▶ 5X Novex TBE Buffer

- ▶ 5 µm Filter Tube
- ▶ 6% Novex TBE PAGE Gel, 1.0 mm, 10 well (1 per 2 sample run)
- ▶ 70% Ethanol, room temperature
- ▶ 100% Ethanol, -15° to -25°C
- ▶ Amplified cDNA Construct (50 µl)
- ▶ Clean Scalpels
- ▶ DNA Loading Dye
- ▶ High Sensitivity DNA Chip
- ▶ Pellet Paint NF Co-Precipitant (Optional)
- ▶ Ultra Pure Ethidium Bromide 10mg/ml

Preparation

- ▶ Remove the Illumina-supplied consumables from -15° to -25°C storage and thaw on ice.
- ▶ Briefly centrifuge the thawed Illumina-supplied consumables at 3,000 rpm for 5 seconds, then place them on ice.

Dilute 10X Gel Elution Buffer

- 1 Dilute the 10X Gel Elution Buffer in a separate, sterile, nuclease-free tube. Multiply each reagent volume by the number of samples being prepared. Make 10% extra reagent if you are preparing multiple samples.

Reagent	Volume (µl)
10X Gel Elution Buffer	30
Ultra Pure Water	270
Total Volume per Sample	300

- 2 Gently pipette the entire volume up and down to mix thoroughly, then centrifuge briefly.
- 3 Label the tube “1X Gel Elution Buffer”.

[Optional] Dilute Pellet Paint NF Co-Precipitant

This process marks the visualization of the DNA pellet with a removable dye, making it easier to see and track.

- 1 Dilute the Pellet Paint NF Co-Precipitant in a separate, sterile, nuclease-free, 200 μl PCR tube. Multiply each reagent volume by the number of samples being prepared, plus 10% extra reagent. Prepare enough pellet paint for a minimum of 10 samples to avoid pipetting small volumes.

Reagent	Volume (μl)
1X Pellet Paint NF Co-Precipitant	0.2
Ultra Pure Water	1.8
Total Volume per Sample	2.0

- 2 Gently pipette the entire volume up and down to mix thoroughly, then centrifuge briefly.
- 3 Label the tube "0.1X Pellet Paint".

Run the Gel Electrophoresis

- 1 Determine the volume of 1X TBE Buffer needed. Dilute the 5X TBE Buffer to 1X for use in electrophoresis.
- 2 Assemble the gel electrophoresis apparatus per the manufacturer's instructions.
- 3 Mix 2 μl of Custom Ladder with 2 μl of DNA Loading Dye.
- 4 Mix 1 μl of High Resolution Ladder with 1 μl of DNA Loading Dye.
- 5 Mix all of the amplified cDNA construct, (typically 48–50 μl) with 10 μl of DNA Loading Dye.
- 6 Load 2 μl of mixed Custom Ladder and loading dye in two wells on the 6% PAGE Gel, as shown in Figure 10.
- 7 Load 2 μl of High Resolution Ladder and loading dye in a different well, as shown in Figure 10.
- 8 Load two wells with 25 μl each of mixed Amplified cDNA Construct and loading dye on the 6% PAGE Gel. A total volume of 50 μl should be loaded on the gel.

- 9 Run the gel for 60 minutes at 145 V or until the blue front dye exits the gel. Proceed immediately to the next step.
- 10 Remove the gel from the apparatus.

Recover the Purified Construct


- 1 Open the cassette according to the manufacturer's instructions and stain the gel with Ethidium Bromide (0.5 $\mu\text{g}/\text{ml}$ in water) in a clean container for 2–3 minutes.
- 2 Place the gel breaker tube into a sterile, round-bottom, nuclease-free, 2 ml microcentrifuge tube.

Figure 9 Place 0.5 ml Tube into 2 ml Tube



- 3 View the gel on a Dark Reader transilluminator or a UV transilluminator.
The following figure shows gel analysis of human brain small RNA library. The Custom Ladder consists of three dsDNA fragments 145 bp, 160 bp, and 500 bp. Sequencing can be conducted on individual bands or from pooled bands. The 147 nt band primarily contains mature microRNA generated from approximately 22 nt small RNA fragments. A second, 157 nt band containing piwi-interacting RNAs, as well as some microRNAs and other regulatory small RNA molecules, is generated from approximately 30 nt RNA fragments.

Figure 10 Small RNA Library from Human Brain Total RNA Samples

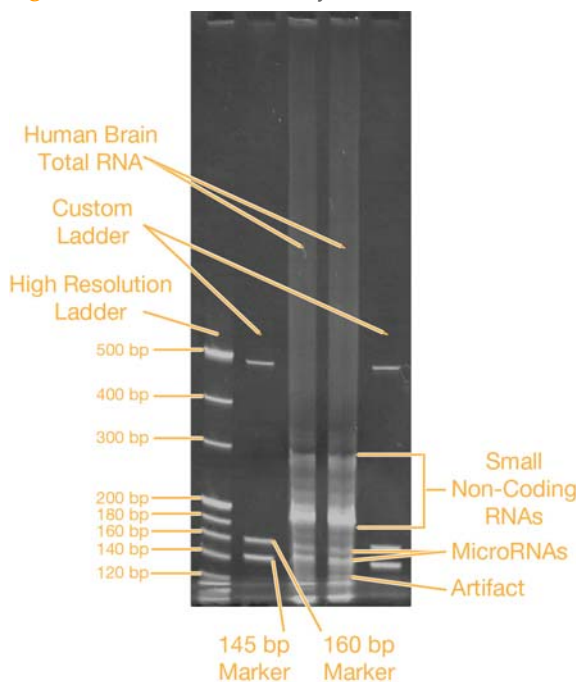

NOTE

The voltage and run time can vary with different electrophoresis equipment. Optimize the running time so that the 145 bp band from the Custom Ladder is close to the bottom of the gel.

- Using a clean scalpel, cut out the bands corresponding to approximately the adapter-ligated constructs derived from the 22 nt and 30 nt small RNA fragments. MicroRNAs often vary in length, often called iso-mirs. The tighter the band selection, the tighter size distribution of the final microRNA representation.

Align the razor blade with the top of the 160 bp band of the Custom Ladder, then with the bottom of the 145 bp band of the Custom Ladder. Excise the gel fragment by connecting these cuts on the sides.

The band containing the 22 nt RNA fragment with both adapters are a total of 147 nt in length. The band containing the 30 nt RNA fragment with both adapters are 157 nt in length.

- Place the band of interest into the 0.5 ml Gel Breaker tube from step 2.

- 6 Centrifuge the stacked tubes at 14,000 rpm in a microcentrifuge for 2 minutes at room temperature to move the gel through the holes into the 2 ml tube. Ensure that the gel has all moved through the holes into the bottom tube.
- 7 Add 300 μ l of Gel Elution Buffer to the gel debris in the 2 ml tube.
- 8 Elute the DNA by rotating or shaking the tube at room temperature for at least 2 hours. the tube can be rotated overnight, if desired.
- 9 Transfer the eluate and the gel debris to the top of a 5 μ m filter.
- 10 Centrifuge the filter for 2 minutes at 14,000 rpm.
- 11 Add 2 μ l of glycogen, 30 μ l of 3M NaOAc, 2 μ l of 0.1X Pellet Paint (optional) and 975 μ l of pre-chilled -15° to -25°C 100% ethanol.
- 12 Immediately centrifuge at 14,000 rpm for 20 minutes on a benchtop microcentrifuge at 4°C .



NOTE

The precipitation mix can be incubated at -80°C for 20–30 minutes, if desired.

- 13 Remove and discard the supernatant, leaving the pellet intact.



NOTE

If the pellet becomes loose, centrifuge at 14,000 rpm at room temperature for 2 minutes.


- 14 Wash the pellet with 500 μ l of room temperature 70% ethanol.
- 15 Centrifuge at 14,000 rpm at room temperature for 2 minutes.
- 16 Remove and discard the supernatant, leaving the pellet intact.
- 17 Dry the pellet by placing the tube, lid open, in a 37°C heat block for 5–10 minutes or until dry.
- 18 Resuspend the pellet in 10 μ l Resuspension Buffer.

Validate the Library

Illumina recommends performing the following quality control analysis on your sample library.

- 1 Load 1 μl of the resuspended construct on an Agilent Technologies 2100 Bioanalyzer using a DNA specific chip such as the DNA-1000 or High Sensitivity DNA chip.
An example of a library prepared using the TruSeq Small RNA Sample Preparation Protocol is shown below with typical results from human brain total RNA.

Figure 11 DNA 1000 Chip Trace of the Final Library from a Human Brain Total RNA sample

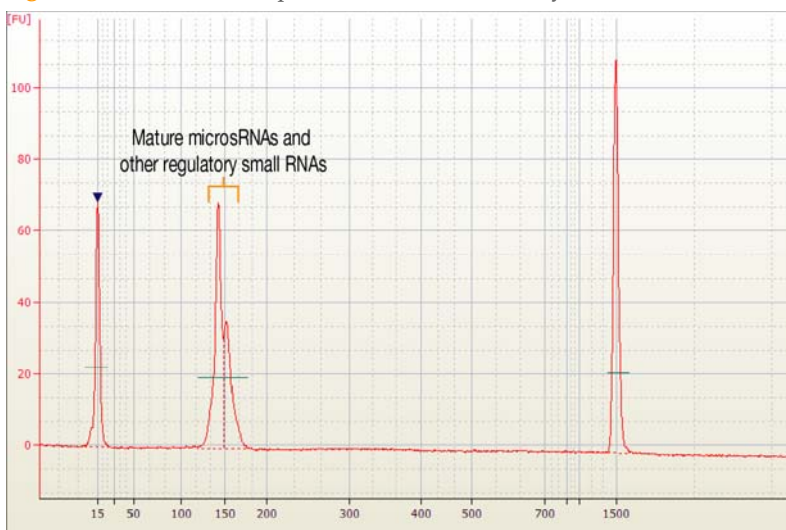

- 2 Check the size, purity, and concentration of the sample.



NOTE

For clustering, use the total of all the molarities from the BioAnalyzer. All peaks create clusters, even if they are adapter dimer, other small RNA, etc. For example, if there are two peaks, add the molarity of each peak. If there are three peaks, add the molarity of the three peaks together. For more information, see the *cBot User Guide*.

DNA Template Storage

Illumina recommends storing prepared DNA template at a concentration of 10 nM.

Adjust the concentration for your prepared DNA samples (or pools of samples) to 10 nM using Tris-HCl 10 mM, pH 8.5. For long-term storage of DNA samples at a concentration of 10 nM, add Tween 20 to the sample to a final concentration of 0.1% Tween. This helps to prevent adsorption of the template to plastic tubes upon repeated freeze-thaw cycles, which would decrease the cluster numbers from a sample over time.

Indexes

Table 4 TruSeq Small RNA Sample Prep Index Sequences

Index	Sequence	Index	Sequence	Index	Sequence
RPI1	ATCACG	RPI17	GTAGAG	RPI33	TCATTC
RPI2	CGATGT	RPI18	GTCCGC	RPI34	TCCCGA
RPI3	TTAGGC	RPI19	GTGAAA	RPI35	TCGAAG
RPI4	TGACCA	RPI20	GTGGCC	RPI36	TCGGCA
RPI5	ACAGTG	RPI21	GTTTCG	RPI37	GCCGCG
RPI6	GCCAAT	RPI22	CGTACG	RPI38	GCCTTA
RPI7	CAGATC	RPI23	GAGTGG	RPI39	GCTCCA
RPI8	ACTTGA	RPI24	GGTAGC	RPI40	GGCACA
RPI9	GATCAG	RPI25	CTAGCT	RPI41	GGCCTG
RPI10	TAGCTT	RPI26	CTAGCT	RPI42	TCTACC
RPI11	GGCTAC	RPI27	CTATAC	RPI43	TGAATG
RPI12	CTTGTA	RPI28	CTCAGA	RPI44	TGCCAT
RPI13	AGTCAA	RPI29	CTGCTG	RPI45	TGCTGG
RPI14	AGTTCC	RPI30	TAATCG	RPI46	TGGCGC
RPI15	ATGTCA	RPI31	TACAGC	RPI47	TTCGAA
RPI16	CCGTCC	RPI32	TATAAT	RPI48	TTCTCC

Technical Assistance

For technical assistance, contact Illumina Customer Support.

Table 5 Illumina General Contact Information

Illumina Website	http://www.illumina.com
Email	techsupport@illumina.com

Table 6 Illumina Customer Support Telephone Numbers

Region	Contact Number
North America toll-free	1.800.809.ILMN (1.800.809.4566)
United Kingdom toll-free	0800.917.0041
Germany toll-free	0800.180.8994
Netherlands toll-free	0800.0223859
France toll-free	0800.911850
Other European time zones	+44.1799.534000
Other regions and locations	1.858.202.ILMN (1.858.202.4566)

MSDSs

Material safety data sheets (MSDSs) are available on the Illumina website at <http://www.illumina.com/msds>.

Product Documentation

If you require additional product documentation, you can obtain PDFs from the Illumina website. Go to <http://www.illumina.com/support/documentation.ilmn>. When you click on a link, you will be asked to log in to iCom. After you log in, you can view or save the PDF. To register for an iCom account, please visit <https://icom.illumina.com/Account/Register>.

Illumina, Inc.

9885 Towne Centre Drive

San Diego, CA 92121-1975

+1.800.809.ILMN (4566)

+1.858.202.4566 (outside North America) techsupport@illumina.com

www.illumina.com